

The suture-pulley method for endolumenal triangulation in endoscopic submucosal dissection

Endoscopic submucosal dissection (ESD) is a time-consuming and technically demanding technique [1–3]. The main difficulty is the lack of triangulated countertraction with current endoscopes [4]. To improve speed and efficacy of the procedure, an intriguing pulley method using dental floss together with endoscopic clips has recently been described [5]. However, current clip technology is unlikely to provide a robust and dependable anchor for this “pulley” technique.

To create a more stable pulley mechanism, we used a novel endoscopic suturing device (Overstitch, Apollo-Endosurgery, Austin, Texas, USA; **Fig. 1**). The device consists of a suture with an anchor/needle threaded through one endoscopic working channel. The anchor can be linked to a curved suturing-arm manipulated via a system-handle on the proximal end of a dual-channel therapeutic gastroscope (**Video 1**). We believe the use of this system could greatly facilitate ESD by providing endolumenal triangulation and retraction (**Fig. 2**).

In an anesthetized 45-kg pig, hypothesized gastric lesions ($n = 2$) were marked by mucosal burns (diameter 3 cm). After lifting the area with saline, a circumferential mucosal incision was performed using a standard needle knife. With the suturing device a suture was first endolumenally anchored at an anterior gastric fold (**Fig. 3**), distal from the lesion. A second bite was placed through the lateral proximal edge of the specimen and the anchor/needle, serving as a lifting retainer, was released. To generate triangulation, another endolumenal pulley was created (**Fig. 4**) at the contralateral mucosal edge. Both suture tails were withdrawn through the mouth and separately clamped with a hemostat. An isolated tip needle knife (IT-knife, Olympus, Center Valley, Pennsylvania, USA)

Video 1

The curved suturing-arm and the anchor/needle are manipulated via a system-handle mounted onto the proximal end of the endoscope (endoscopic and external view).



Fig. 1 The distal part of the endoscopic suturing device, mounted onto the tip of a dual-channel endoscope.

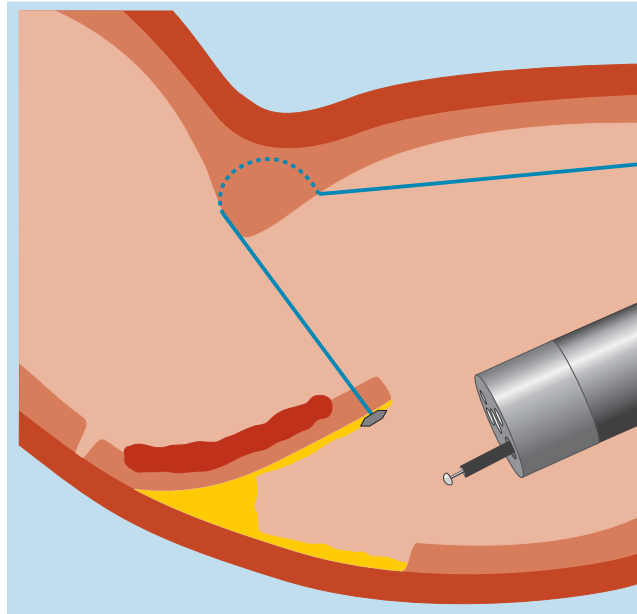


Fig. 2 The anchor/needle of the device has been released and serves as secure lifting retainer for the endolumenal suture pulley, providing endolumenal triangulation and retraction.

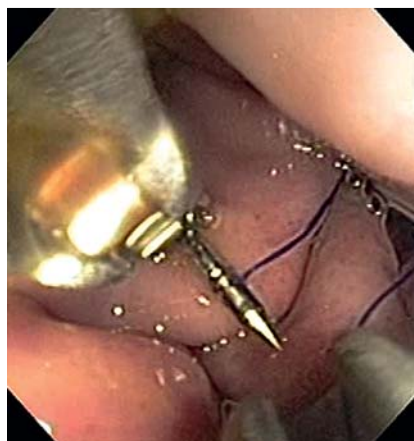


Fig. 3 The anchor/needle is linked to the curved suturing arm, before the suture will be endolumenally anchored to an anterior gastric fold.

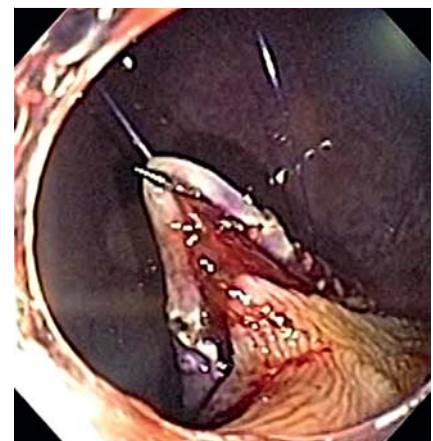


Fig. 4 After a second bite through the lateral proximal edge of the hypothesized lesion the anchor/needle has been released and serves as secure lifting retainer.

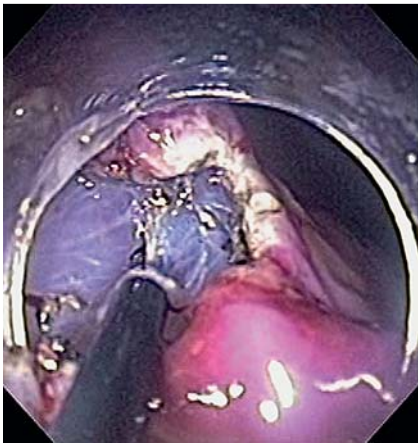


Fig. 5 Triangulation and retraction provided by the suture-pulleys facilitates endoscopic submucosal dissection.

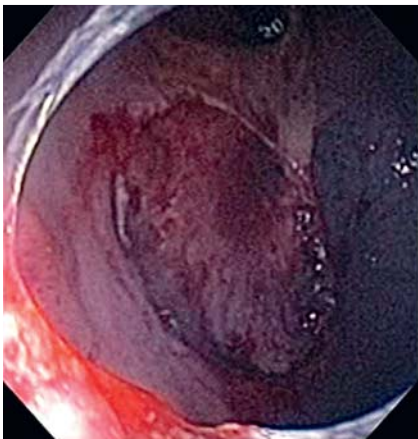


Fig. 6 The hypothesized gastric lesion has been resected (retroflexed view).

was used for submucosal dissection while alternately pulling on the sutures to lift and retract the specimen (● Fig. 5). All suture-pulleys ($n = 4$) were easily created within 5.3 ± 0.3 min. Subsequent submucosal dissections were successfully performed in 34.0 ± 1.4 min, without perforations (● Fig. 6, ● Video 2).

Video 2

Creation of an endolumenal suture pulley to enable triangulation and retraction for endoscopic submucosal dissection.

The use of an endoscopic suturing device could facilitate dissection of large superficial gastrointestinal lesions by enabling endolumenal triangulation.

Endoscopy_UCTN_Code_TTT_1AO_2AG

Competing interests: None

E. Rieder¹, K. I. Makris¹, D. V. Martinec², L. L. Swanström²

¹ Minimally Invasive Surgery Program, Legacy Health, Portland, Oregon, USA

² Gastrointestinal and Minimally Invasive Surgery Division, The Oregon Clinic, Portland, Oregon, USA

References

- 1 Deprez PH, Bergman JJ, Meisner S et al. Current practice with endoscopic submucosal dissection in Europe: position statement from a panel of experts. *Endoscopy* 2010; 42: 853–858
- 2 Neuhaus H, Costamagna G, Deviere J et al. Endoscopic submucosal dissection (ESD) of early neoplastic gastric lesions using a new double-channel endoscope (the “R-scope”). *Endoscopy* 2006; 38: 1016–1023
- 3 Imagawa A, Okada H, Kawahara Y et al. Endoscopic submucosal dissection for early gastric cancer: results and degrees of technical difficulty as well as success. *Endoscopy* 2006; 38: 987–990
- 4 Lee SH, Gromski MA, Derevianko et al. Efficacy of a prototype endoscope with two deflecting working channels for endoscopic submucosal dissection: a prospective comparative, ex vivo study. *Gastrointest Endosc* 2010; 72: 155–160
- 5 Li CH, Chen PJ, Chu HC et al. Endoscopic submucosal dissection with the pulley method for early gastric cancer (with video). *Gastrointest Endosc* 2011; 73: 163–167

Bibliography

DOI 10.1055/s-0030-1256774

Endoscopy 2011; 43: E319–E320

© Georg Thieme Verlag KG Stuttgart · New York · ISSN 0013-726X

Corresponding author

E. Rieder

Minimally Invasive Surgery Program

Legacy Health

1040 NW 22nd Avenue

Suite 560

Portland

97210 OR

USA

erwin.rieder@meduniwien.ac.at